

RADCELF User Guide

Rev	Date	Description
1	20160826	init
6	20200819	new-style clock diagram, spell out CLK/TRG cmds
7	20200920	support GPS ntp, web counters page
10	20201028	FAT.

Document created using OpenOffice.Org www.openoffice.org.

This document and D-TACQ Software comprising platform Linux port, Linux kernel modules and most applications are released under GNU GPL/FDL:

Document:

Copyright (c) 2016 Peter Milne, D-TACQ Solutions Ltd.

Permission is granted to copy, distribute and/or modify this document under the terms of the GNU Free Documentation License, Version 1.2, with no Invariant Sections, no Front-Cover Texts, and no Back-Cover Texts.

Software:

Copyright (C) 2016 Peter Milne, D-TACQ Solutions Ltd.

This program is free software; you can redistribute it and/or modify it under the terms of the GNU General Public License version 2 as published by the Free Software Foundation.

This program is distributed in the hope that it will be useful, but WITHOUT ANY WARRANTY; without even the implied warranty of MERCHANTABILITY or FITNESS FOR A PARTICULAR PURPOSE. See the GNU General Public License for more details.

You should have received a copy of the GNU General Public License along with this program; if not, write to the Free Software Foundation, Inc., 59 Temple Place, Suite 330, Boston, MA 02111-1307 USA

Table of Contents

1	Introduction.....	4
1.1	Scope.....	4
1.2	References.....	4
1.3	Software concept.....	4
2	AD9854 DDS.....	5
2.1	Virtual Devices.....	5
2.1.1	Top level directory for RADCELF.....	5
2.1.2	One virtual file per register.....	5
2.1.3	Knobs accessed from site service.....	5
2.1.4	Example Site Service Usage.....	5
2.1.5	Socket with complete low level emulation.....	6
2.1.6	Recommended Scripting Style.....	6
2.1.7	Help.....	7
2.1.8	Register Dumps.....	7
2.1.9	Load/Restore state.....	7
2.1.10	Strobe.....	8
2.2	Web page.....	9
3	AD9512 CLKD.....	10
3.1	Virtual Devices.....	10
3.1.1	Top level directory for RADCELF.....	10
3.1.2	One virtual file per register.....	10
3.1.3	Knobs accessed from site service.....	10
3.1.4	Example Site Service Usage.....	10
3.1.5	Help.....	10
4	Voltage Monitor and DIO.....	12
4.1	DIO direction.....	12
5	Boot Time Initialisation.....	12
6	Test routines.....	13
6.1	Sets some default clocks.....	13
6.2	Set a single chirp.....	13
7	Remote Scripting.....	14
7.1	Monitoring After Chirp : Web pages:.....	15
7.2	Monitoring CLKD.....	16
7.3	Monitoring Chirp.....	17
7.3.1	OPI.....	17
7.3.2	Web.....	18
7.4	Remote monitoring.....	19
7.5	Hooking RADCELF outputs on ZYNQ FPGA.....	20
7.5.1	Clock Signals.....	20
7.5.2	Trigger Signals.....	20
8	GNSS Integration.....	21
8.1	GNSS Unit.....	21
8.2	Theory Of Operation.....	21
8.3	Time Multiplexing.....	22
8.4	GPSNTP.....	23
8.4.1	Customisation.....	23
8.4.2	Ublox Initialisation.....	23

8.5	GPS RESET.....	23
8.6	ubxtool.....	23
	ubxtool(1) is provided to interrogate the u-blox, and it can apparently change defaults.....	23
8.6.1	Web Diagnostics : GPSPMON.....	24
8.6.2	Web Diagnostics GPSNTP.....	25
8.7	Clock conditioning to ONEPPS.....	26
8.7.1	Before Tuning.....	26
8.7.2	After Tuning.....	26
8.7.3	Finally.....	27
8.7.4	Automated Frequency Tuning.....	27
8.7.4.1	From Boot.....	27
8.7.4.2	Start a chirp.....	27
8.7.4.3	Initial Local Clock Tuning.....	28
8.7.4.4	<i>Fine</i> Clock Tuning.....	29
8.8	Synchronized Chirp.....	29
8.8.1	Trigger_at.....	29
8.8.2	Radcelf-Chirp-Init.....	30
8.8.3	Test Case Example.....	30
8.8.4	Turnkey Example.....	31
8.8.5	Boot time Configuration.....	32
8.8.6	In-Data Instrumentation.....	32
8.8.7	Factory Test.....	33
8.8.7.1	On Each Box.....	33
8.8.7.2	On Master Box.....	33
8.8.7.3	On Host.....	33
8.8.7.4	On Master Box.....	33
8.8.7.5	On Host.....	34
8.8.7.6	Compare instrumentation on two boxes:.....	35
9	Appendix.....	37
9.1	Software Install.....	37
9.1.1	Install Fresh Release.....	37
9.1.2	U-Boot settings.....	37
10	Appendix: Production Self-Tests.....	38
10.1	DDS.....	38
10.2	Aux DIO.....	38
10.3	USB.....	38
10.4	Check all signal outputs.....	38
11	Appendix: GPS Master/Slave Systems.....	39
11.1	Hardware.....	39
11.2	Once-per-boot commands.....	39
11.2.1	Master.....	39
11.2.2	Slave.....	39
11.3	Streaming Data.....	39
11.4	Start the run:.....	39
12	Appendix: AD9854 Quickref.....	40

1 Introduction

1.1 Scope

Covers software control of RADCELF.

RADCELF has the following programmable devices:

- 1) AD9854 DDS : ddsA, ddsB, ddsC
- 2) AD9512 CLKD chips clkdA, clkdB
- 3) AD7417 temperature and slow ADC
- 4) 8 bit slow DIO buffer.

1.2 References

- 1) RADCELF Block Diagram
- 2) AD9854 Data Sheet
- 3) [AD9854 Quick Ref](#)
- 4) AD512 Data Sheet
- 5) 4GUG

1.3 Software concept

Each device is represented by a device driver that presents every register as a virtual file or “knob”. The knobs have meaningful names and are set with simple ascii strings. Where possible, knobs are read/write. These features make for easy local scripting. Scripting languages available on the ACQ400 series include : shell, TCL, python.

In addition, it's ACQ400 convention to present every user-controllable knob on a “site service” where it's accessible by connecting a TCP socket to a well-known port. This makes writing a remote automation script extremely easy. The site service may also be accessed locally using the **set.site** command.

Then, to examine and optionally set the complete state of the device, virtual files are provided to dump / load all the registers in the device. This information is also presented in a dynamic web page for easy monitoring.

2 AD9854 DDS

2.1 Virtual Devices

2.1.1 Top level directory for RADCELF

```
ls /dev/radcelf
clkdA clkdB ddsA ddsB ddsC
```

2.1.2 One virtual file per register

```
cd /dev/radcelf/ddsA
ls [A-Z][A-Z]*
CR      DFR      FTW1      FTW2      IPDMR      POTW1      POTW2      QDACR      QPDMR      RRCR      SKRR      UCR
```

2.1.3 Knobs accessed from site service

<i>Chip</i>	<i>Site</i>	<i>Port</i>	<i>Local Command</i>	<i>Remote Command</i>
ddsA	4	4224	set.site 4	nc ACQ 4224
ddsB	5	4225	set.site 5	nc ACQ 4225
ddsC	6	4226	set.site 6	nc ACQ 4226

2.1.4 Example Site Service Usage

Shows a get followed by a set. It's a good idea to check that the set worked, at least in debug by following it up with another get. Or refer to the web page.

```
acq1001_068> set.site 4
FTW1
1000000000000
FTW1=1100000000000
FTW1
1100000000000

Baadd=B0409
FTW1
0900000000000
```

So either way you can set FTW1, however, apart from being less legible, “Baadd” is really inefficient, because not only are 6 commands required to complete the word, each command has to write the full 7 byte command..

2.1.5 *Socket with complete low level emulation*

Ports 4244, 4245, 4346 emulate the Baadd protocol directly, this is provided so that customer's existing client software may run directly.

Configuration:

```
acq1001_068> cat /etc/inetd.radcelf.conf
4244 stream tcp nowait root set.Baadd set.Baadd 4
4245 stream tcp nowait root set.Baadd set.Baadd 5
4346 stream tcp nowait root set.Baadd set.Baadd 6
```

Example:

```
a-host> nc acq1001_068 4244
B0411
B0500
B0600
B0700
B0800
B0900
```

Equivalent to

```
nc acq1001_068 4224
FTW1=1100000000000
```

2.1.6 *Recommended Scripting Style*

Convenience commands are provided to easy local scripting:

set.ddsA	FTW1	0123456789abc
set.clkB	UPDATE	01

2.1.7 Help

```
acq1001_068> set.site 4 help2
BPSK          : rw
               0 FPGA Enable BPSK
CR            : rw
               [7,4] Control Register
DFR           : rw
               [4,6] Delta Frequency Register
FTW1          : rw
               [2,6] Frequency Tuning Word #1
FTW2          : rw
               [3,6] Frequency Tuning Word #2
IPDMR         : rw
               [8,2] I Path Digital Multiplier Register
OSK           : rw
               0 FPGA Enable OSK
POTW1         : rw
               [0,2] Phase Offset Tuning Word Register #1
POTW2         : rw
               [1,2] Phase Offset Tuning Word Register #2
QDACR         : rw
               [B,2] Q DAC Register 2 Bytes
QPDMR         : rw
               [9,2] Q Path Digital Multiplier Register
RRCR          : rw
               [6,3] Ramp Rate Clock Register
SKRR          : rw
               [A,1] Shaped On/Off Keying Ramp Rate Register
UCR           : rw
               [5,4] Update Clock Rate Register
strobe        : rw
               0 manually strobes update if required
strobe_mode   : rw
               0 0:manual 1:self 2:group (hit strobe to assert group)
help          :
help          :
help2         :
               /usr/share/doc/acq400_help0:help2
```

2.1.8 Register Dumps

```
acq1001_068> cat /proc/driver/ad9854/ddsA/rare
0000
0000
11000000000000
00000000000000
00000000000000
000000000
000000
000f0041
0000
0000
00
0000
```

2.1.9 Load/Restore state

```
cat /proc/driver/ad9854/ddsA/rare >/mnt/local/ddsA_saved_state
... later
```

```
cat /mnt/local/ddsA_saved_state > /proc/driver/ad9854/ddsA/rare
```

2.1.10 *Strobe*

AD9854 requires the IOUD signal to clock register settings through to the device.

Each DDS driver provides the **strobe_mode** knob to control this operation.

Values for **strobe_mode** are:

0 : **SPI_STROBE_NONE**

no action, a separate write to the **strobe** knob pulses IOUD

1: **SPI_STROBE_SELF**

automatic IOUDD pulse after each command [default]

2: **SPI_STROBE_GROUP**

ddsA, ddsB constitute a group, in this mode, a write to the **strobe** knob pulses IOUD on both dds devices to enable synchronous update

2.2 Web page.

Shows complete register state of all 3 DDS, + measured output frequency

The screenshot shows the web interface for the acq1001_153 device. The browser window is titled "acq1001_153 - Mozilla Firefox". The address bar shows "acq1001_153/d-tacq/#DDS". The navigation bar includes tabs for Home, System, Firmware, FPGA, Temperature, Power, Top, Interrupts, acq400.0, and acq400.1. The DDS tab is selected, displaying a table of registers and their values for three DDS units (A, B, and C).

	DDS A	DDS B	DDS C
* DDS	---	---	---
+ FIN	20.00E+6	--	--
* INTCLK	300.0E+6	300.0E+6	300.0E+6
/ FREQ	18.76E+6	21.10E+6	23.44E+6
0 POTW1	0000	0000	0000
1 POTW2	0000	0000	0000
2 FTW1	0.062500 100000000000	0.070312 120000000000	0.078125 140000000000
3 FTW2	0.000000 000000000000	0.000000 000000000000	0.000000 000000000000
4 DFR	000000000000	000000000000	000000000000
5 UCR	00000000	00000000	00000000
6 RRCR	000000	000000	000000
7 CR	X15 004f0041	X15 004f0041	X15 004f0041
8 IPDMR	0000	0000	0000
9 QPDMR	0000	0000	0000
a SKRR	00	00	00
b QDACR	0000	0000	0000

At the bottom of the interface, there is a status bar showing "acq1001_153" and "Thu Jun 1 15:02:44 UTC 2017". There are also buttons for "Refresh?" (checked) and "Done".

3 AD9512 CLKD

3.1 Virtual Devices

3.1.1 Top level directory for RADCELF

```
ls /dev/radcelf
clkdA clkdB ddsA ddsB ddsC
```

3.1.2 One virtual file per register

```
acq1001_068> cd /dev/radcelf/clkdA/
acq1001_068> ls [A-Z][A-Z]*
CSPD      DFA4      DIV0      DIV2      DIV4      LVDS3      LVPECL0   LVPECL2   UPDATE
DBP4      DFS4      DIV1      DIV3      FUNPS     LVDS4      LVPECL1   SCPC
```

3.1.3 Knobs accessed from site service

Chip	Site	Port	Local Command	Remote Command
clkdA	7	4227	set.site 7	nc ACQ 4227
clkdB	8	4228	set.site 8	nc ACQ 4228

3.1.4 Example Site Service Usage

Shows a get followed by a set. It's a good idea to check that the set worked, at least in debug by following it up with another get. Or refer to the web page.

```
acq1001_068> set.site 4
FTW1
100000000000
FTW1=110000000000
FTW1
110000000000
```

3.1.5 Help

```
acq1001_068> set.site 7
help2
CSPD      : rw
[45 1] Clocks Select Power Down
DBP4      : rw
[34 1] Delay Bypass 4
DFA4      : rw
[36 1] Delay Fine Adjust 4
DFS4      : rw
[35 1] Delay Full Scale 4
DIV0      : rw
[4A 2] Divider 0 8000 => Bypass
DIV1      : rw
```

	[4C 2]	Divider 1	8000 => Bypass
DIV2		:	rw
	[4E 2]	Divider 2	8000 => Bypass
DIV3		:	rw
	[50 2]	Divider 3	8000 => Bypass
DIV4		:	rw
	[52 2]	Divider 4	8000 => Bypass
FUNPS		:	rw
	[58 1]	FUNCTION Pin and Sync	
LVDS3		:	rw
	[40 1]	LVDS CMOS Out 3	
LVDS4		:	rw
	[41 1]	LVDS CMOS Out 4	
LVPECL0		:	rw
	[3D 1]	LVPECL Out 0	
LVPECL1		:	rw
	[3E 1]	LVPECL Out 1	
LVPECL2		:	rw
	[3F 1]	LVPECL Out 2	
SCPC		:	rw
	[0 1]	Serial Port Control Configuration	
UPDATE		:	rw
	[5A 1]	Update Registers	

4 Voltage Monitor and DIO

Knobs available on site 3.

d? : dio bit

in? : analog inputs

temp?: temperature.

```
acq1001_153> get.site 3
help
ai1
ai2
ai3
ai4
ai5
ai6
ai7
ai8
d0
d1
d2
d3
d4
d5
d6
d7
temp
temp2
```

4.1 DIO direction

Default: out, set by modifying file on boot as follows (script in /mnt/local/rc.user).

```
acq1001_153> cat /dev/gpio/CELF/.direction.d0
out
acq1001_153> echo in > /dev/gpio/CELF/.direction.d0
```

5 Boot Time Initialisation

/usr/local/init/RAD-CELF-init

Enables the DDS devices, configures a 25MHz source clock and sets the DDS to run internally at 300MHz.

6 Test routines

6.1 Sets some default clocks

`/usr/local/CARE/radcelf-init-123`

Configures ddsA , ddsB, ddsC with test frequencies. Use Web page to confirm it's working.

6.2 Set a single chirp

shell script runs on ACQ1001, sets single chirp

```
#!/bin/sh
#
# SETTING KAKA'AKOS CHIRP
#
# Set AD9854 clock remap to 25 MHz
export PATH=$PATH:/usr/local/bin
set.ddsC      CR      004C0041
set.ddsC      FTW1     1AAAAAAAAAAAA
# Program AD9512 secondary clock to choose 25 MHz from the AD9854 remap
set.clkdB     CSPD     02
set.clkdB     UPDATE   01
# Program the chirp using Kaka'ako parameters
set.site 2 ddsA_upd_clk_fpga 1
set.ddsA      CR      004F0061
set.ddsA      FTW1     172B020C49BA
set.ddsA      DFR      0000000021D1
set.ddsA      UCR      01F01FDO
set.ddsA      RRCR     000001
set.ddsA      IPDMR    0FFF
set.ddsA      QPDMR    0FFF
set.ddsA      CR      004C8761
# Set the trigger
set.site 2 ddsA_upd_clk_fpga 0
# lera_acq_setup
# we assume a 25MHz from ddsC
# trigger from site 3 ddsA
set.site 1 trg 1,3,1
set.site 1 clk 1,3,1
set.site 1 hi_res_mode 1
# 25 MHz/4 = 6.25MHz / 512 = SR 12207
set.site 1 CLKDIV 4
```

7 Remote Scripting

D-TACQ offers a host side api “HAPI”. This brings all the site services together in one consistent object API. https://github.com/petermilne/acq400_hapi/test_apps

Example below “radcelf-chirp-init.py” sets up a chirp on either ddsA or ddsB

Note, it's basically identical to the shell script example, but with a richer capability. HAPI scripts may also be run on the embedded system, which includes a full Python 3 from 2020.

```
def init_chirp(uut, idds):
# SETTING KAKA'AKOS CHIRP
#
# Set AD9854 clock remap to 25 MHz
    dds = uut.ddsA if idds == 0 else uut.ddsB

    uut.ddsC.CR      = '004C0041'
    uut.ddsC.FTW1    = FTW1(1.0/12.0)
# Program AD9512 secondary clock to choose 25 MHz from the AD9854 remap
    uut.clkB.CSPD    = '02'
    uut.clkB.UPDATE  = '01'
# Program the chirp using Kaka'ako parameters
    set_upd_clk_fpga(uut, idds, '1')
    dds.CR           = '004F0061'
    dds.FTW1         = '172B020C49BA'
    dds.DFR          = '0000000021D1'
    dds.UCR          = '01F01FD0'
    dds.RRCR         = '000001'
    dds.IPDMR        = '0FFF'
    dds.QPDMR        = '0FFF'
    dds.CR           = '004C8761'
    set_upd_clk_fpga(uut, idds, '0')

# Set the trigger
# lera_acq_setup
# we assume a 25MHz from ddsC
# trigger from site 3 ddsA
    uut.s1.trg       = '1,3,1'
    uut.s1.clk       = '1,3,1'
    uut.s1.hi_res_mode = '1'
# 25 MHz/4 = 6.25MHz / 512 = SR 12207
    uut.s1.CLKDIV    = '4'
# create an object instance and init_chirp
init_chirp(acq400_hapi.RAD3DDS("acq1001_181"), 0)
```

7.1 Monitoring After Chirp : Web pages:

The screenshot displays the web interface for the acq1001_181 device. The browser window is titled 'acq1001_181 - Mozilla Firefox'. The address bar shows 'acq1001_181/d-tacq/#DDS'. The navigation menu includes tabs for Home, System, Firmware, FPGA, Temperature, Power, Top, Interrupts, and acq400.0. The 'acq400.0' tab is selected, showing a table of DDS parameters for three channels (A, B, C). The table includes parameters like FIN, INTCLK, FREQ, FTW1, FTW2, DFR, UCR, RRCR, CR, IPDMR, QPDMR, SKRR, and QDACR. The bottom status bar shows 'acq1001_181', 'Wed Jun 28 16:19:05 UTC 2017', and buttons for 'Refresh?' and 'Done'.

	--- DDS A ---	--- DDS B ---	--- DDS C ---
* DDS			
+ FIN	25.00E+6	--	--
* INTCLK	300.0E+6	300.0E+6	300.0E+6
/ FREQ	27.30E+6	27.30E+6	25.00E+6
0 POTW1	0000	0000	0000
1 POTW2	0000	0000	0000
2 FTW1	0.090500 172b020c49ba	0.090500 172b020c49ba	0.083333 155555555555
3 FTW2	0.000000 000000000000	0.000000 000000000000	0.000000 000000000000
4 DFR	0000000021d1	0000000021d1	000000000000
5 UCR	01f01fd0	01f01fd0	00000000
6 RRCR	000001	000001	000000
7 CR	X12 004c8761	X12 004c8761	X12 004c0041
8 IPDMR	0fff	0fff	0000
9 QPDMR	0fff	0fff	0000
a SKRR	00	00	00
b QDACR	0000	0000	0000

acq1001_181 Wed Jun 28 16:19:05 UTC 2017 Refresh? Done

7.2 Monitoring CLKD

acq1001_181 - Mozilla Firefox

File Edit View History Bookmarks Tools Help

acq1001_181 x MultiMon x New Tab x acq1001_060 x RAD_CELF: Main R x +

acq1001_181/d-tacq/#CLKD

Home System Firmware FPGA Temperature Power Top Interrupts acq400.0

acq400.1 acq400.2 DDS **CLKD**

reg	clkdA	clkdB
CSPD	00	02
DBP4	01	01
DFA4	00	00
DFS4	00	00
DIV0	1100	0000
DIV1	1100	0000
DIV2	1100	0000
DIV3	1100	0000
DIV4	1100	0000
FUNPS	00	00
LVDS3	01	00
LVDS4	00	02
LVPECL0	00	00
LVPECL1	00	00
LVPECL2	0a	0a
SCPC	10	10
UPDATE	00	00

acq1001_181 Wed Jun 28 16:19:19 UTC 2017 ☒ Refresh? Done

Web page shows current CLKD register settings.

7.3 Monitoring Chirp

7.3.1 OPI

Users with cs-studio get a colour mimic

ACQ400_LAUNCHER.opi acq1001ctr.opi radcelfctr.opi

acq1001_194RADCELF TRIPLE DDS COUNTERS

CLK.d0	CLK.d1	CLK.d2	CLK.d3	CLK.d4	CLK.d5	CLK.d6
3.277E7 Hz	2.227E7 Hz	6.250E6 Hz	2.500E7 Hz	2.729E7 Hz	2.729E7 Hz	0.000 Hz
1106531938212	7520947280570	7473394833046	8442160684521	6352218040149	7136081824685	0
EXT	MB	ADC ISR	DDSClk	ddsA	ddsB	ddsC

TRG.d0	TRG.d1	TRG.d2	TRG.d3	TRG.d4
0.000 Hz	0.000 Hz	0.000 Hz	5.000 Hz	5.000 Hz
0	0	0	1E4	1E4
EXT	MB	S1	Chirp A	Chirp B

EVT.d0	EVT.d1	EVT.d2	EVT.d3
0.000 Hz	0.000 Hz	0.000 Hz	5.000 Hz
0	0	0	1E4
EXT	MB	S1	S2

SYN.d0	SYN.d1	SYN.d2	SYN.d3
0.000 Hz	0.000 Hz	0.000 Hz	5.000 Hz
0	0	0	1E4
EXT	MB	ADC OSR	S2

** These counters are good to about 50MHz. Higher frequencies, or rapidly fluctuating frequencies will NOT record correctly.

7.3.2 Web

NEW from 2020 - 09 -20 : web display shows the counters without need for cs-studio:

The web page style is very basic, but it does update dynamically.

1.1 SIGNAL	CLK.d0	CLK.d1	CLK.d2	CLK.d3	CLK.d4	CLK.d5	CLK.d6
1.2 FREQ	32.77E+6	22.27E+6	6.250E+6	25.00E+6	27.30E+6	27.30E+6	25.00E+6
1.3 COUNT	1.489E+12	1.012E+12	953.2E+9	1.136E+12	99.93E+9	99.88E+9	91.53E+9
1.4 FUNCTION	EXT	MB	ADC ISR	DDSClk	ddsA	ddsB	ddsC

2.1 SIGNAL	TRG.d0	TRG.d1	TRG.d2	TRG.d3	TRG.d4	TRG.d5	TRG.d6
2.2 FREQ	0.000	0.000	0.000	5.000	5.000	1.000	0.000
2.3 COUNT	0	0	0	16.90E+3	16.89E+3	45.43E+3	0
2.4 FUNCTION	EXT	MB	S1	Chirp A	Chirp B	GPSx	GPSy

7.4 Remote monitoring

The frequency counters are aliased on site 2 with meaningful names:

```
[pgm@hoy4 acq400_hapi_tests]$ nc acq1001_181 4222
*SIG*
SIG:DDS:A:CHIRP:COUNT 595852
SIG:DDS:A:CHIRP:FREQ 0
SIG:DDS:A:FREQ 0
SIG:DDS:B:CHIRP:COUNT 77397
SIG:DDS:B:CHIRP:FREQ 0
SIG:DDS:B:FREQ 0
SIG:DDS:C:FREQ 0
SIG:DDS:INP:FREQ 25004591
```

The counters may be cleared from this knob:

```
clear_counts 1
```

Clearing the counts is useful to track “number of chirp cycles from start”.

The DDS and CLKD system may be restored to power up state:

```
RADCELF_init 1
```

7.5 Hooking RADCELF outputs on ZYNQ FPGA

7.5.1 Clock Signals

Signals appearing on the clock bus. The most common usage is to link a clock source to the ADC in site 1. eg

- `set.site 1 clk=1,1,1` # source from the MBCLOCK (ACQ435 default mode)
- `set.site 1 clk=1,3,1` # source from DDSCLK
- `set.site 1 clk=1,6,1` # source from ddsC

Name	Clock Bus	Comment
EXT	d0	Front panel clock
MB	d1	Motherboard Clock MBCLK
ADC	d2	ADC modulator clock
DDSCLK	d3	DDS source clock (clkdB output)
ddsA	d4	
ddsB	d5	
ddsC	d6	

For full understanding of motherboard clock routing, please refer to CLKTREE OPI

7.5.2 Trigger Signals

Signals appearing on the TRG bus. Likely use cases:

- `set.site 1 trg=1,0,1` # set external start trigger
- `set.site 1 event0=1,3,1` # embedded timing event on ChirpA
- `set.site 1 RGM:DX=d3` # Burst Mode, trigger on ChirpA

Name	TRG Bus	Comment
EXT	d0	Front panel trigger
SOFT	d1	Soft trigger
GPG2	d2	GPG output
ChirpA	d3	DDSA Chirp trigger
ChirpB	d4	DDSB Chirp trigger
PPS	d5	GPS PPS Output (1Hz)
PPS2	d6	GPS PPS2 Output (100Hz)
GPG7	d7	GPG output
GPG: Gate Pulse generator, programmable intervals from trigger		

8 GNSS Integration

Feature set available from 2020-09-21

8.1 GNSS Unit

uBlox RCB-F9T-0-01 precision time module may be integrated with RADCELF

The GNSS unit provides an NMEA feed to the ACQ1001 on `devttySP1` and a ONE-PPS signal that is mapped by the FPGA to TRG.d5 and GPIO453

8.2 Theory Of Operation

This document describes the FPGA changes and software methods used to demonstrate GPS synchronisation in the RAD-CELF of the ACQ435 Digitiser to within a small fraction of the sample clock.

The GPS RAD-CELF synchronisation involves frequency synchronisation across multiple RAD-CELF modules by measuring the frequency of the local oscillator after passing through the Clock Remapping DDS (DDS-C). This frequency is then adjusted to precisely 25 MHz.

To do this the FPGA counts the number clock cycles between the PPS pulses from the GPS module. This is then averaged over 10, 30 and 100 seconds to obtain up to 0.01 Hz resolution on the frequency. The FTW1 on the remapping DDS is adjusted up or down until the target 25 MHz frequency is reached. The precision of the FTW on the DDS device allows this precision to be reached. The limiting factors are GPS PPS precision, and both GPS and Oscillator drift in both time and temperature.

The FPGA logic provides the Oscillator count from DDS-C and software provides this count and the average of 10, 30 and 100 seconds.

The script **radcelf-tune-pps.py** is provided to adjust the DDS FTW to achieve 25 MHz to within 0.02 Hz accuracy

Running **radcelf-tune-pps.py --fine=1**, program continuously after the main script to attempt to maintain the frequency over a long period, during the shot, if necessary.

Once the Frequency has been adjusted the system can then be started using the new FPGA logic that synchronises the Chirp start to the GPS PPS logic.

This achieves synchronous chirp generation but the ACQ435 is a sigma-delta ADC which divides down the system clock by 512 to achieve the sample clock,

this means that another change to the FPGA is needed to adjust the “phase” of this sample clock divider to achieve ADC synchronisation across multiple devices.

The problem is that the current setup results in a sample frequency of

$25\text{MHz}/(4 \times 512)$ of 12207.03 kHz. This means that the ADC sample point is constantly rotating with respect to the GPS PPS signal.

The method chosen was to use a frequency that is a multiple of 512Hz rather than the nominal 25 MHz. This requires the frequency of DDS-C to move to 24.999936 MHz. This changes the default sample rate of 12207.03 Hz to exactly 12207 Hz.

With this integer number of samples per second the GPS PPS signal can then be used to reset the

phase of the 512 clock divider to the nearest oscillator clock. This achieves a 1/512 skew between two ACQ435 digitisers synchronised this way.

The FPGA was changed so that prior to starting a capture the ADC divider synchronises to every PPS pulse. Once a capture is started the synchronisation is disabled and subject to any drift between the clocks.

Due to the ADC pipeline there is a 40 sample settling time for the FIR filter in the ADC before data capture can commence, this is a minor issue as it is normally several seconds before the ADC is triggered.

This method is a proof of concept to show synchronous sampling of the ADC if the frequency change is an issue further mechanisms would be explored.

The script **radcelf-tune-pps.py** takes an optional user-supplied DDSCLK frequency as first argument [default 25000000]. The script runs by default in a mode `--best=1`, this will adjust the supplied frequency to the nearest multiple of 512Hz. Users can disable this feature by running `--best=0`.

8.3 *Time Multiplexing*

RCB-F9T actually has two PPS outputs. PPS1 is used for the main synchronization procedure below. PPS2 is set on boot to run at 100Hz. It's not currently used, but we suggest it could be the basis of a Time Domain Multiplex system, where multiple transmitters share the same frequency, but are allocated time slots. For example, if one second is divided into 100 timeslots, then Radar A could be set to chirp on PPS2#33 aka Slot 33 and Radar B could be set to chirp on PPS2#34 aka Slot 34 and in this way they don't interfere.

We have a mechanism that allows a radar to select a given 1PPS edge; this isn't in the current firmware, but this mechanism could be extended to select a given 100PPS edge.

8.4 GPSNTP

Enable by setting optional package : 99-custom_gpsntp-2009201746.tgz or newer

8.4.1 Customisation

A default ntp customisation file is provided:

/usr/local/CARE/GPSNTP/ntp.conf, this is copied into place at /etc/ntp.conf on boot

Should this not be sufficient, the user is free to create a custom ntp.conf, to be installed on boot:

/mnt/local/ntp.conf, copied to /etc/ntp.conf on boot

8.4.2 Ublox Initialisation

On boot, system is informed of the presence of RCB-F9T (or other UBLOX device) with this setting. For additional information, please see /usr/local/init/custom_gpsntp-README

```
acq1001_450> cat /mnt/local/sysconfig/acq400.sh
GPS_UBX=y
```

This triggers some default processing (see custom_gpsntp.init) , resetting the UBLOX and setting TP2 to 100 Hz (For Time Multiplex possibility: 8.3)

```
if [ "$GPS_UBX" != "x" ]; then
    if [ -e /mnt/local/ublox.conf ]; then
        /mnt/local/ublox.conf
    else
        gps_reset
        sleep 10
        ubx_set_tp2
        sleep 5
    fi
fi
```

This behaviour may be modified by creating a local file /mnt/local/ublox.conf

8.5 GPS RESET

example: reset ON, reset OFF:

```
acq1001_427> set.site 2 gps_reset 1
```

8.6 ubxtool

ubxtool(1) is provided to interrogate the u-blox, and it can apparently change defaults.

8.6.1 Web Diagnostics : GPSPMON

The “gpsmon” link on the home page launches an interactive gpsmon window.

The screenshot displays the GPSPMON web interface in a Mozilla Firefox browser. The browser address bar shows the URL `10.12.197.20/d-tacq/#Home`. The main content area shows a terminal window with the following data:

```

tcp://localhost:2947 NMEA0183>
Time: 2020-09-20T18:39:39.000Z Lat: 55 46.682390' N Lon: 4 05.954220' W
Cooked TPV

GLGSV GAGSV GBGSV GNGLL GNRMC GNVTG GNGGA GNOSA GPGSV

Sentences

Ch PRN Az El S/N Time: 183939.00 Time: 183939.00
0 5 187 50 8 Latitude: 5546.68239 N Latitude: 5546.68239
1 7 60 27 0 Longitude: 00405.95422 W Longitude: 00405.95422
2 8 39 9 0 Speed: 0.119 Altitude: 101.4
3 13 273 72 38 Course: 149.23 Quality: 1 Sats: 12
4 15 281 37 36 Status: A FAA: A HDOP: 0.80
5 18 305 24 41 MagVar: RMC Geoid: 50.6
6 20 322 4 19 GGA
7 23 322 1 0
8 27 7 8 36 Mode: A3 ...s: 5 13 15 18 2 UTC: RMS:
9 28 130 32 27 DOP: H=0.80 V=1.00 P=1.28 MAJ: MIN:
10 30 74 55 25 TOFF: 0.069758828 ORI: LAT:
11 5 187 50 0 PPS: LON: ALT:
GSA + PPS GST
(52) $GNGLL,5546.68239,N,00405.95422,W,183939.00,A,A*61
  
```

Below the terminal window, there are links for Online Documents and Module Calibration files.

Online Documents

Local customisation files in /mnt/loc

- [/mnt/local/rc.user](#)
- [/mnt/local/sysconfig/acq400.sh](#)
- [/mnt/local/sysconfig/bos.sh](#)
- [/mnt/local/sysconfig/epics.sh](#)
- [/mnt/local/sysconfig/site-1-peers](#)
- [/mnt/local/sysconfig/transient.init](#)
- [/tmp/u-boot_env](#)
- [gpsmon](#)

Module Calibration files :


<http://www.d-tacq.com/>

8.6.2 Web Diagnostics GPSNTP

The GPSNTP tab shows results on “ntp -p” updated on a 3s schedule

The key figure of merit is PPS jitter, showing 0.009 msec in the screenshot below:


The number after the date is the ntp run time, normally it will need a few minutes to stabilize.

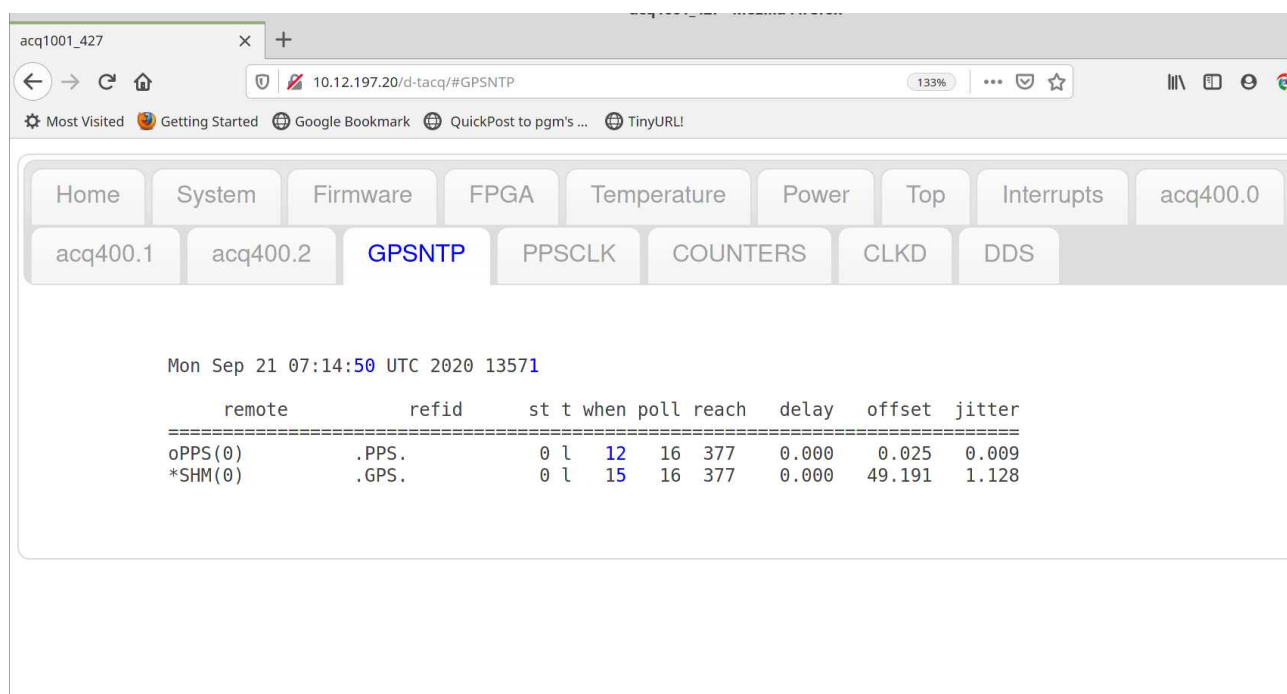

8.7 Clock conditioning to ONEPPS


FPGA hardware maintains a count of DDS-C output, latched every ONEPPS. The intention is that DDS-C can be tuned to an exact number of cycles per ONEPPS interval so that the DDS clock is exactly tuned to GNSS. The tuning may be conducted over a long interval.

8.7.1 Before Tuning

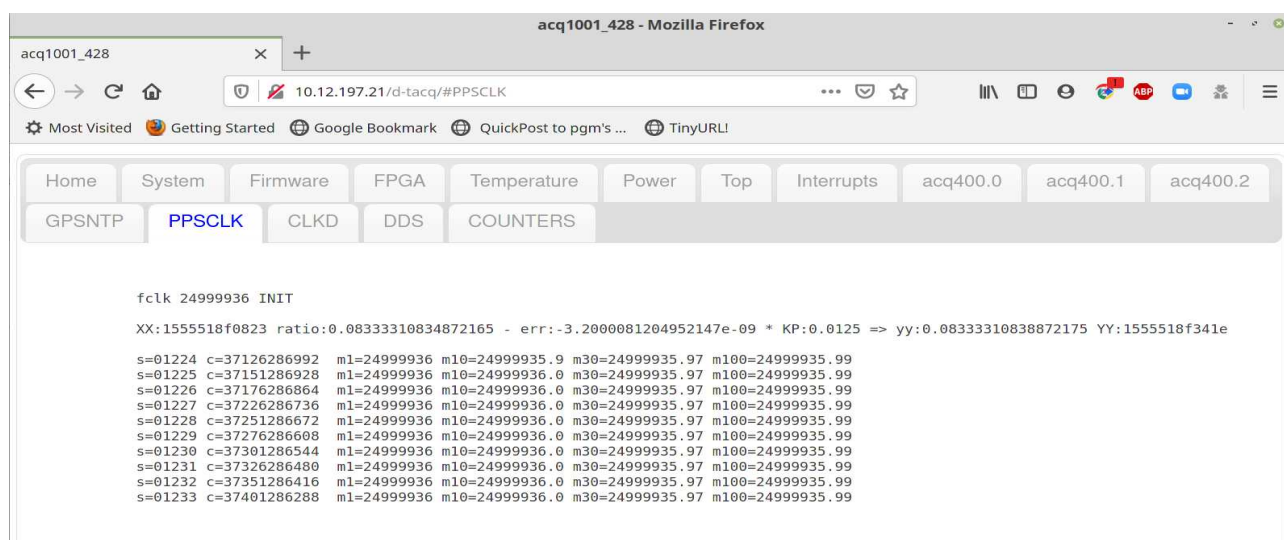


8.7.2 After Tuning

DDS-C was tweaked from 15555555555 to 15555d8a555.

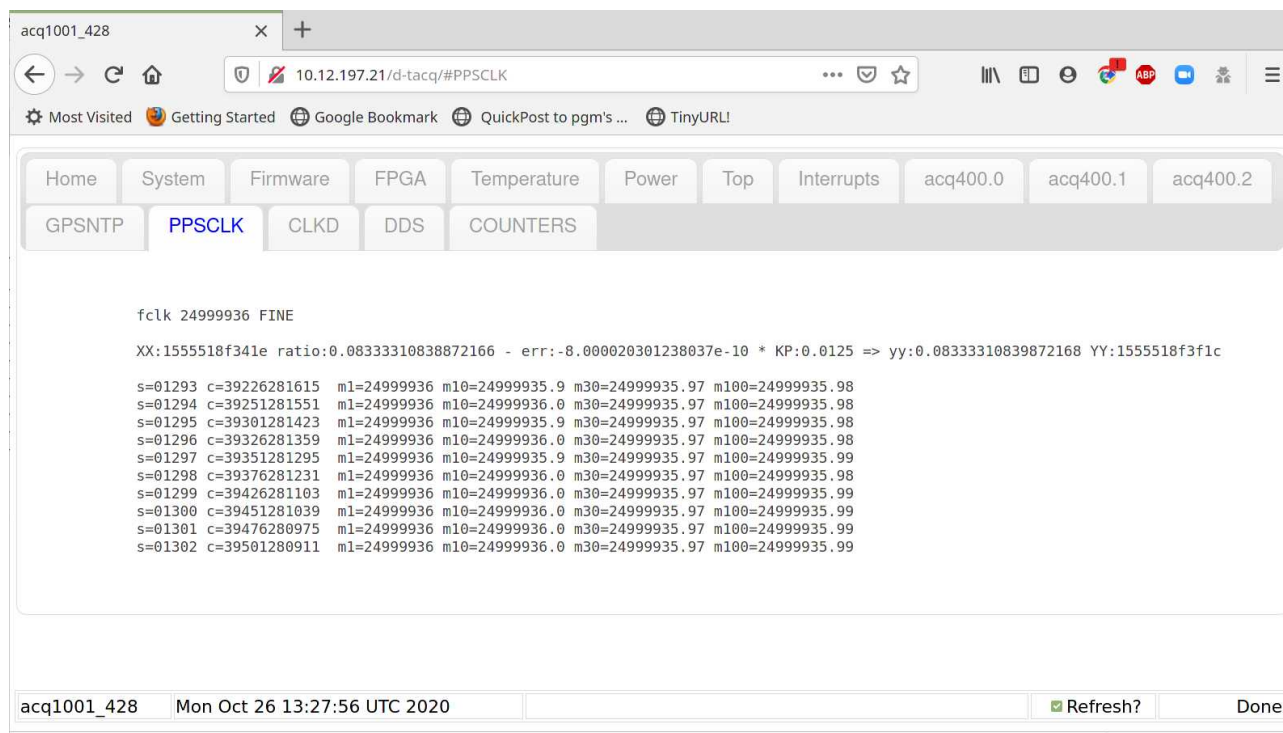

8.7.3 Finally

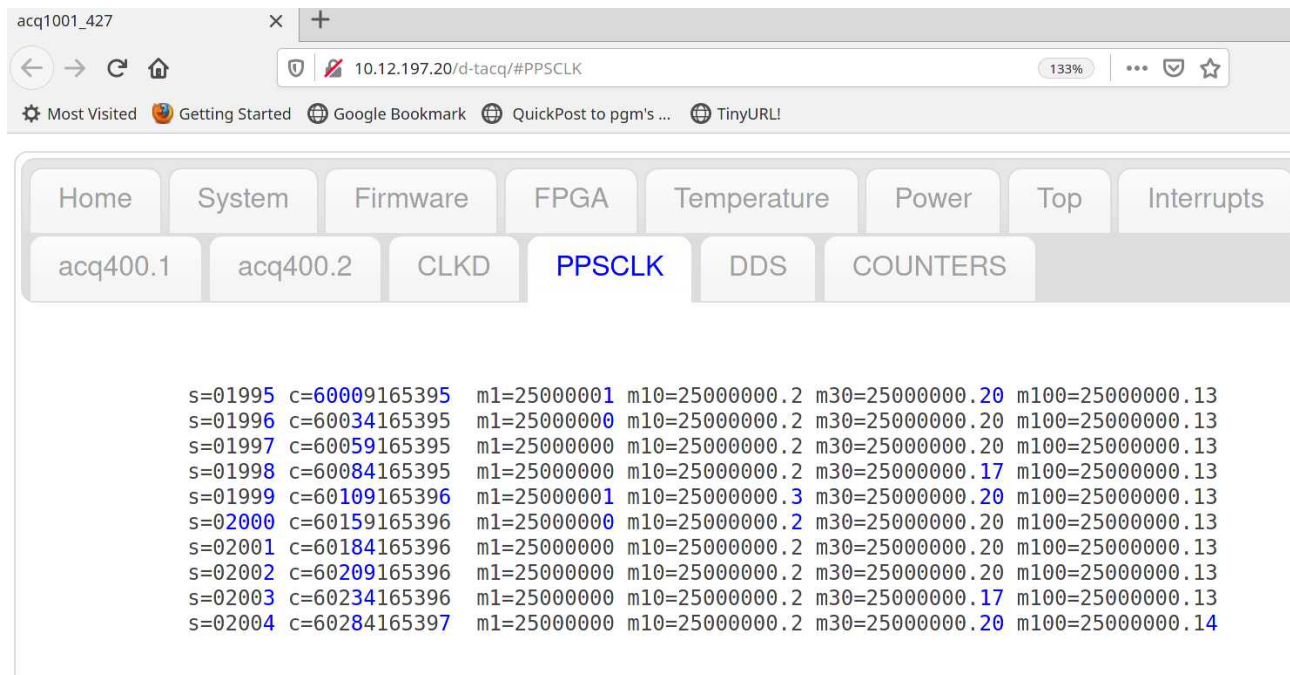

8.7.4 Automated Frequency Tuning

8.7.4.1 From Boot

Possible to run **radcelf-tune-pps.py** from `//mnt/local/rc.user`.

8.7.4.2 Start a chirp

```
acq1001_427> /usr/local/HAPI/test_apps/radcelf-chirp-init.py localhost
test:0 PASS SIG:TRG_S2:FREQ 0.000 SIG:TRG_S3:FREQ 0.000
```

8.7.4.3 Initial Local Clock Tuning

radcelf-tune-pps.py [--best[=1] DDSCLK] :Runs once and terminates

```
acq1001_427> radcelf-tune-pps.py
control m1
XX:155555555555 ratio:0.08333333333333215 - err:-3.6e-07 * KP:0.05 =>
yy:0.08333335133333215 YY:155555a2a48a
control m1
XX:155555a2a48a ratio:0.08333335133333009 - err:-4e-07 * KP:0.05 =>
yy:0.08333337133333009 YY:155555f88ac5
control m1
XX:155555f88ac5 ratio:0.08333337133332819 - err:1.2e-07 * KP:0.05 =>
yy:0.08333336533332819 YY:155555dec5b3
control m10
XX:155555dec5b3 ratio:0.08333336533332769 - err:-7.200000002980232e-08 *
KP:0.05 => yy:0.0833333689333277 YY:155555ee3bf0
control m10
XX:155555ee3bf0 ratio:0.08333336893332444 - err:5.200000002980232e-08 * KP:0.05
=> yy:0.08333336633332443 YY:155555e31135
control m10
XX:155555e31135 ratio:0.08333336633332422 - err:3.200000002980232e-08 * KP:0.05
=> yy:0.08333336473332421 YY:155555dc31fd
control m10
XX:155555dc31fd ratio:0.08333336473332409 - err:1.200000002980232e-08 *
KP:0.05 => yy:0.08333336413332408 YY:155555d99e48
control m100
XX:155555d99e48 ratio:0.08333336413332404 - err:-5.999999940395355e-09 *
KP:0.05 => yy:0.08333336443332404 YY:155555dae822
```

NB: this is a simple proportional control servo; likely end-users will be able to come up with a better algorithm. Note the count converging to 25Mhz exactly over all time periods..

The last state of radcelf-tune-pps.py is presented on the PPSCLK web page.

- XX: Current 48bit FTW
- ratio: Current FTW as a ratio
- error: difference with desired value
- KP : proportional gain constant.
- yy: Next value as a ratio
- YY: Next 48 bit FTW.

The control algorithm doesn't claim to be the best. In particular, the very low Kp value was found by experiment. The author's suspicion is that because we're actually controlling a ratio, our control function is not a linear gain, but rather a reciprocal gain and therefore applying a linear constant doesn't work as expected. This should be a nice control problem to solve optimally.

8.7.4.4 *Fine Clock Tuning*

radcelf-tune-pps.py --fine=1 : fine tuning that could run continuously.

8.8 *Synchronized Chirp*

8.8.1 *Trigger_at*

Starts a trigger on a given GPS second.

Usage:

trigger_at +N : trigger in +N seconds (actually, only useful for single UUT)

trigger_at TIME_T : trigger at this TIME_T (in the future)

trigger_at today HH:MM[:SS] [HH:MM ...] Wall Clock Style

- +N style is only helpful when testing a single UUT (think: delays on network)
- TIME_T style is ideal for script controlled testing (radcelf-chirp-init use it)
- Wall Clock style can be used for turnkey systems

8.8.2 Radcelf-Chirp-Init

radcelf-chirp-init.py [--opts] [uuts]

- default uut : localhost
- radcelf-chirp-init can set up several U.
- User can chose whether to use a central script setting many uuts, or to configure each uut individually.

```
acq1001_427> radcelf-chirp-init.py --help
usage: radcelf-chirp-init.py [-h] [--test TEST] [--debug DEBUG]...

radcelf-chirp-init

positional arguments:
  uuts                uut

optional arguments:
  -h, --help            show this help message and exit
  --test TEST            set number of tests to run
  --debug DEBUG          1: trace 2: step
  --noverify NOVERIFY   do not verify (could be waiting gps)
  --ddsX DDSX            ddsA=1, ddsB=2, ddsA+ddsB=3
  --gps_sync GPS_SYNC   synchronize with GPSPPS >1: autotrigger at + gps_sync s
  --chirps_per_sec CHIRPS_PER_SEC
                        chirps per second
  --stop                --stop uuts : stop chirp and quit [no value]
  --trigger_adc_dx TRIGGER_ADC_DX
                        trigger ACQ on ddsA or ddsB or dX [X=0,1,2,3,4,5,6]
  --init_trigger         --init_trigger : configure trigger only
```

- By default radcelf-chirp-init.py with no args will run exactly as per the original version, setting up ddsA, ddsB chirps at 5Hz, soft triggered on localhost.
- --ddsX=1 : init ddsA only
- --ddsX=2 :init ddsB only
- --chirps_per_sec=N may be used to set other chirp rates, to the limits of available parameters.
- --gps_sync N, N> : will autotrigger at +N seconds
- --gps_sync -1 : will configure for autotrigger, but leave the actual time of trigger for others to set up
- use SITECLIENT_TRACE to show the commands
- use --debug=1 to trace operation (prints names of functions on entry/exit)
- use --debug=2 to step operation (user breakpoint at start/end of every function.
- --stop [uuts] : STOP the chirp and capture on UUTS.

8.8.3 Test Case Example

```
SITECLIENT_TRACE=1 \
radcelf-chirp-init.py --chirps_per_sec=10 --gps_sync=5 \
acq1001_427 acq1001_428
```

- configure 2 UUTs to run 10 chirps per second, triggering 5s in the future

8.8.4 Turnkey Example

All units are configured to boot turnkey, and to restart every hour:

Embed in a boot script eg //mnt/local/radcelf-turnkey-boot and call in the background from //mnt/local/rc.user

NB: this example is a little contrived. Users will probably do better, but it shows the concept:

Example uses at(1) to control setups and captures ahead of time, so the setup is complete and the capture is armed ahead of the precise trigger time.

```
#!/bin/sh
# radcelf-turnkey-boot, run a capture on the hours for the workday morning

sleep 300                # allow GPSNTP to settle

radcelf-tune-pps.py       # tune the clock (once)

radcelf-tune-pps.py --fine=1 & # leave the fine tuning on in the background

# trigger every hour on the hour
trigger_at today 07:00 08:00 09:00 10:00 11:00 12:00

# setup radcelf-chirp-init to reinitialise 5 minutes before hand.
echo radcelf-chirp-init.py --chirps_per_sec=10 | at 06:55
echo radcelf-chirp-init.py --chirps_per_sec=10 | at 07:55
echo radcelf-chirp-init.py --chirps_per_sec=10 | at 08:55
echo radcelf-chirp-init.py --chirps_per_sec=10 | at 09:55
echo radcelf-chirp-init.py --chirps_per_sec=10 | at 10:55
echo radcelf-chirp-init.py --chirps_per_sec=10 | at 11:55
```

On the HOST computer, there could be a similar arrangement to capture the data

```
echo acq400_stream.py --time=60min --output=UUT.0700.dat UUT | at 06:55
echo acq400_stream.py --time=60min --output=UUT.0800.dat UUT | at 07:55
echo acq400_stream.py --time=60min --output=UUT.0900.dat UUT | at 08:55
echo acq400_stream.py --time=60min --output=UUT.1000.dat UUT | at 09:55
echo acq400_stream.py --time=60min --output=UUT.1100.dat UUT | at 10:55
echo acq400_stream.py --time=60min --output=UUT.1200.dat UUT | at 11:55
```

All normal alternatives to HOST-PULL streaming are available.

For example, ACQ1001 can still remote mount an NFS disk and stream locally to the local mount

eg assuming an nfs mount /nfs

```
echo timeout -s 3600 nc localhost 4210 > /nfs/UUT.0700.dat | at 06:55
echo timeout -s 3600 nc localhost 4210 > /nfs/UUT.0700.dat | at 07:55
echo timeout -s 3600 nc localhost 4210 > /nfs/UUT.0700.dat | at 08:55
echo timeout -s 3600 nc localhost 4210 > /nfs/UUT.0700.dat | at 09:55
echo timeout -s 3600 nc localhost 4210 > /nfs/UUT.0700.dat | at 10:55
echo timeout -s 3600 nc localhost 4210 > /nfs/UUT.0700.dat | at 11:55
```

8.8.5 Boot time Configuration

```
acq1001_427> cat /mnt/local/sysconfig/transient.init
COOKED=0 NSAMPLES=100000 NCHAN=8 TYPE=LONG
transient PRE=2000 POST=2000 OSAM=1 DEMUX=1 SOFT_TRIGGER=1

# always trigger on CHIRPA
set.site 1 trg=1,3,1
# GPS sync
set.site 1 sync=1,0,1
# IOC not up yet, have to go low..
#set.site 0 SIG:SRC:SYNC:0=PPS
set.sys /dev/acq400.0.knobs/sig_src_route_sync_d0 3

/usr/local/CARE/make_spad_id
set.site 0 spad=1,4,0
set.site 0 spad1_us_clk_d1 1
set.site 0 spad1_us 1,3,1

spad2_monitor
spad3_monitor

run0 1
make-ch-server
```

8.8.6 In-Data Instrumentation

- Per sample, we have:
 - N columns of AI data, 32 bit
 - 24 bit signed ADC value {31:8}
 - 8 bit channel ID {7:0} 0x20, 0x21, 0x22.. 0x27
 - 4 columns Scratchpad (SPAD), each unsigned
 - SPAD[0] : Sample number
 - SPAD[1] : Clock count (6.25Mhz clock)
 - SPAD[2] : EVENT LATCH Count : sample count at PPS edge
 - SPAD[3] : KTIME_T, updated at 1kHz. Kernel ktime_t is 64 bit, we encode 32 bits as follows:
 - 20 bits time_t seconds {31:12}
 - 12 bits milliseconds {7:0} actual range : 0..999

The firmware includes a handy tool to check KTIME_T:

```
acq1001_427> /usr/local/CARE/spad3_timestamp_check
Wed Oct 21 18:37:36 UTC 2020 5f907ff0 0x07ff014d

Where :
5f907ff0      is the current time_t
07ff014d      is the KTIME_T, with 20 bit seconds, followed by msec.
```

8.8.7 Factory Test

8.8.7.1 On Each Box

The text box represents a terminal session. Leave it running:

```
radcelf-tune-pps.py  
radcelf-tune-pps.py --fine=1
```

8.8.7.2 On Master Box

```
acq1001_427> export SITECLIENT_TRACE=1  
acq1001_427> radcelf-chirp-init.py --debug=1 --stop acq1001_427 acq1001_428
```

8.8.7.3 On Host

```
nc acq1001_427 53667 | pv > acq1001_427.5.dat
```

```
nc acq1001_428 53667 | pv > acq1001_428.5.dat
```

nb: nc UUT SPYPORT is shown for convenience, a real system might use **acq400_stream2.py** and it might also run on the UUT to stream to an NFS mount.

We propose using the SPYPORT to receive data rather than the STREAMPORT (4210), since opening the SPYPORT doesn't affect the start up sequence in the way that connecting to STREAMPORT does (ie it does not cause the capture system to ARM and possibly run); in otherwords, it's easier to set up a complex sequence, and the single program **radcelf-chirp-init.py** is then responsible for the entire start up sequence.

8.8.7.4 On Master Box

```
radcelf-chirp-init.py --chirps_per_sec=5 --gps_sync=5 acq1001_427 acq1001_428  
  
sleep 60  
  
radcelf-chirp-init.py --stop acq1001_427 acq1001_428
```

8.8.7.5 On Host

- First, look at AI data [0..7,8] and sample count

```
[peter@andros ~]$ hexdump -e '12/4 "%08x," "\n"' acq1001_427.5.dat | cut -d, -f1-9 | head
30753820,007f1121,00816822,00760023,0076d124,00000f25,009a7826,00760327,00000001
338cb620,007e4621,00810722,0075a523,00768824,ffffab25,009a2b26,0070fb27,00000002
31680720,007a1921,007e3022,00722523,0073a124,ffff3025,00969626,00630e27,00000003
33306c20,00786121,007d0722,0070eb23,00727024,ffefd25,00954426,005ce527,00000004
31d5df20,0074ee21,007a9422,006e3f23,00700a24,ffe8225,00926926,00525227,00000005
```

- Second : look at Instrumentation Data [8,9,10,11,12]
- SPAD0 : Sample count : starts at zero, increments in 1's
- SPAD1: ADC modulator clock count (6.25MHz). Starts at 0x5000+ ???
- SPAD2 : SAMPLE count at Event Latch (Event1=CHIRP), starts at zero
- SPAD3 : KTIME_T

```
hexdump -e '12/4 "%08x," "\n"' acq1001_427.5.dat | cut -d, -f9,10,11,12 | less
00000001,00005139,00000000,082b5003
00000002,00005339,00000000,082b5003
00000003,00005539,00000000,082b5003
00000004,00005739,00000000,082b5003
00000005,00005939,00000000,082b5003
...
0000098b,00136539,00000000,082b50cb
0000098c,00136739,00000000,082b50cb
0000098d,00136939,00000989,082b50cb
0000098e,00136b39,00000989,082b50cb
0000098f,00136d39,00000989,082b50cb
```

8.8.7.6 Compare instrumentation on two boxes:

```
dt100@andros ~]$ cat bin/pasty
paste \
<(hexdump -e '12/4 "%08x," "\n"' $1 | cut -d, -f9,10,11,12)\
<(hexdump -e '12/4 "%08x," "\n"' $2 | cut -d, -f9,10,11,12)
```

- **Analysis of next page: START**

- 6Mhz clock count at start: 0x50d8, 0x50d9 : remote UUT's agree to 0.16usec.
- Initial count 0x50d0 is the 40 sample initial pipeline
- First PPS Latch is a relic from previous shot, please ignore
- NTP / KTIME-T agrees to 1msec.

- **First Event**

- First event latch value 0x989. This is inserted by SOFTWARE AFTER the event. The event position is found at sample index 0x989, 2441 Decimal.
- Time to first event : $0x989 \Rightarrow 2441 * 512 / 6.25M = 0.200 \text{ s}$
- Time to first event from NTP $\Rightarrow 0xca-0x02 = 200\text{msec}$

- **Second Event**

- Second event latch value 0x1312, This is inserted by SOFTWARE AFTER the event. The event position is found at sample index 0x1312, 4882 decimal.
- Time to second event: $0x1312 \Rightarrow 4882 * 512 / 6.25\text{Mhz} = 0.400\text{s}$
- Time to second event NTP: $0x190 \rightarrow 400\text{msec}$.

A python analysis program is provided to validate over long periods: **radcelf_sync_test.py**

```
pasty acq1001_427.dat acq1001_428.dat | grep -n . | less
```

SampleD, SampleX, 6MHz clocks, PPS Latch, NTP Time

```

1:00000001,000050d8,000eb703,98deb002      00000001,000050d9,000f7f48,98deb003
2:00000002,000052d8,00000000,98deb002      00000002,000052d9,000f7f48,98deb003
3:00000003,000054d8,00000000,98deb002      00000003,000054d9,000f7f48,98deb003
4:00000004,000056d8,00000000,98deb002      00000004,000056d9,000f7f48,98deb003
5:00000005,000058d8,00000000,98deb002      00000005,000058d9,000f7f48,98deb003
6:00000006,00005ad8,00000000,98deb002      00000006,00005ad9,000f7f48,98deb003
7:00000007,00005cd8,00000000,98deb003      00000007,00005cd9,000f7f48,98deb003
8:00000008,00005ed8,00000000,98deb003      00000008,00005ed9,000f7f48,98deb003
9:00000009,000060d8,00000000,98deb003      00000009,000060d9,000f7f48,98deb003

2441:00000989,001360d8,00000000,98deb0ca    00000989,001360d9,00000000,98deb0cb
2442:0000098a,001362d8,00000000,98deb0ca    0000098a,001362d9,00000000,98deb0cb
2443:0000098b,001364d8,00000000,98deb0ca    0000098b,001364d9,00000000,98deb0cb
2444:0000098c,001366d8,00000989,98deb0ca    0000098c,001366d9,00000000,98deb0cb
2445:0000098d,001368d8,00000989,98deb0ca    0000098d,001368d9,00000000,98deb0cb
2446:0000098e,00136ad8,00000989,98deb0ca    0000098e,00136ad9,00000000,98deb0cb
2447:0000098f,00136cd8,00000989,98deb0ca    0000098f,00136cd9,00000000,98deb0cb
2448:00000990,00136ed8,00000989,98deb0cb    00000990,00136ed9,00000000,98deb0cb
2449:00000991,001370d8,00000989,98deb0cb    00000991,001370d9,00000000,98deb0cb
2450:00000992,001372d8,00000989,98deb0cb    00000992,001372d9,00000000,98deb0cb
2451:00000993,001374d8,00000989,98deb0cb    00000993,001374d9,00000000,98deb0cb
2452:00000994,001376d8,00000989,98deb0cb    00000994,001376d9,00000000,98deb0cb
2453:00000995,001378d8,00000989,98deb0cb    00000995,001378d9,00000989,98deb0cb
2454:00000996,00137ad8,00000989,98deb0cb    00000996,00137ad9,00000989,98deb0cc
2455:00000997,00137cd8,00000989,98deb0cb    00000997,00137cd9,00000989,98deb0cc
2456:00000998,00137ed8,00000989,98deb0cb    00000998,00137ed9,00000989,98deb0cc
2457:00000999,001380d8,00000989,98deb0cb    00000999,001380d9,00000989,98deb0cc

4879:0000130f,00266cd8,00000989,98deb192    0000130f,00266cd9,00000989,98deb192
4880:00001310,00266ed8,00000989,98deb192    00001310,00266ed9,00000989,98deb192
4881:00001311,002670d8,00000989,98deb192    00001311,002670d9,00000989,98deb192
4882:00001312,002672d8,00000989,98deb192    00001312,002672d9,00000989,98deb192
4883:00001313,002674d8,00000989,98deb192    00001313,002674d9,00000989,98deb193
4884:00001314,002676d8,00000989,98deb192    00001314,002676d9,00000989,98deb193
4885:00001315,002678d8,00001312,98deb192    00001315,002678d9,00000989,98deb193
4886:00001316,00267ad8,00001312,98deb192    00001316,00267ad9,00000989,98deb193
4887:00001317,00267cd8,00001312,98deb192    00001317,00267cd9,00000989,98deb193
4888:00001318,00267ed8,00001312,98deb192    00001318,00267ed9,00000989,98deb193
4889:00001319,002680d8,00001312,98deb192    00001319,002680d9,00000989,98deb193
4890:0000131a,002682d8,00001312,98deb193    0000131a,002682d9,00000989,98deb193
4891:0000131b,002684d8,00001312,98deb193    0000131b,002684d9,00000989,98deb193
4892:0000131c,002686d8,00001312,98deb193    0000131c,002686d9,00000989,98deb193
4893:0000131d,002688d8,00001312,98deb193    0000131d,002688d9,00000989,98deb193
4894:0000131e,00268ad8,00001312,98deb193    0000131e,00268ad9,00001312,98deb193
4895:0000131f,00268cd8,00001312,98deb193    0000131f,00268cd9,00001312,98deb194
4896:00001320,00268ed8,00001312,98deb193    00001320,00268ed9,00001312,98deb194
4897:00001321,002690d8,00001312,98deb193    00001321,002690d9,00001312,98deb194

```

9 Appendix

9.1 *Software Install*

9.1.1 *Install Fresh Release*

acq400-268-20201012082516 or newer

Customize after install as follows:

```
mv /mnt/packages.opt/35-radcelf* /mnt/packages
mv /mnt/packages.opt/38-custom_hapi-* /mnt/packages
mv /mnt/packages.opt/99-*gpsntp* /mnt/packages
```

9.1.2 *U-Boot settings.*

NB: all units shipped with RADCELF fitted already have this selection, so it's NOT necessary to do it again

Connect serial console

Press <SPACE> within 3s of power up

from the u-boot prompt:

```
u-boot> setenv devicetree_image dtb.d/acq1002r.dtb
u-boot> saveenv
u-boot> boot
```

10 Appendix: Production Self-Tests

10.1 DDS

- run this script: /usr/local/CARE/radcelf-init-123
- Check this result:
- 20MHz becomes 18.75, 21.09 and 23.4 MHz on ddsA, ddsB, ddsC, respectively.

See Web Page 2.2

10.2 Aux DIO

- connect a 16 way header cable from J1 to J2.
- run this script:

```
acq1001_153> /usr/local/CARE/rad_aux_test
loopback J1 to J2
make all dX outputs, active high
OUT:0 0 0 0 0 0 0 0 0 BACK:0 0 0 0 0 0 0 0 PASS 0 0 0 0 0 0 0 0
OUT:1 0 0 0 0 0 0 0 0 BACK:1 0 0 0 0 0 0 0 PASS 2476 0 0 0 0 0 0 0
OUT:0 1 0 0 0 0 0 0 0 BACK:0 1 0 0 0 0 0 0 PASS 0 2478 0 0 0 0 0 0
OUT:0 0 1 0 0 0 0 0 0 BACK:0 0 1 0 0 0 0 0 PASS 0 0 2476 0 0 0 0 0
OUT:0 0 0 1 0 0 0 0 0 BACK:0 0 0 1 0 0 0 0 PASS 0 0 0 2476 0 0 0 0
OUT:0 0 0 0 1 0 0 0 0 BACK:0 0 0 0 1 0 0 0 PASS 0 0 0 0 2485 0 0 0
OUT:0 0 0 0 0 1 0 0 0 BACK:0 0 0 0 0 1 0 0 PASS 0 0 0 0 0 2493 0 0
OUT:0 0 0 0 0 0 1 0 0 BACK:0 0 0 0 0 0 1 0 PASS 0 0 0 0 0 0 2480 0
OUT:0 0 0 0 0 0 0 0 0 BACK:0 0 0 0 0 0 0 0 PASS 0 0 0 0 0 0 0 0
PASS: 9/9 PASS
```

10.3 USB

Connect USB stick and confirm it's available.

It's necessary to set bConfigurationValue to force power up.

```
echo 1 > /sys/bus/usb/devices/1-1.1/bConfigurationValue
mkdir /sd
mount /dev/sda1 /sd
```

10.4 Check all signal outputs

Run the dual chirp and use a scope to monitor (not covered in this guide)

11 Appendix: GPS Master/Slave Systems

SCENARIO: 2 x 16 channel boxes, but only ONE has the RADCELF.

The RADCELF unit M can master the slave system S over HDMI.

11.1 Hardware

Connect SYNC_OUT HDMI on M to SYNC IN HDMI on S.

11.2 Once-per-boot commands

11.2.1 Master

this is already set by default in //mnt/local/rc.user

radcelf-tune-pps.py may be running continuously on your system, but if not, run it for 30s to setup the RADCELF clocks.

```
sync_role_master_radcelf
timeout 30 radcelf-tune-pps.py
```

11.2.2 Slave

This should be set in //mnt/local/rc.user if the system is always going to work in this role

(not set by factory as it prevents the box working turnkey with no additional setup, which is how we like to ship..

```
set.site 0 sync_role slave
```

11.3 Streaming Data

Data is streamed in spy mode, either from an external HOST (in this example), or locally, perhaps to an NFS mount: Set this up on bot boxes.

```
nc UUT 53667 | pv > /dev/null
# or
nc localhost 53667 > /mnt/nfs/file.dat
```

11.4 Start the run:

On MASTER only, substitute network host names for MASTER and SLAVE:

```
radcelf-chirp-init.py --use_dds_on_first_uut_only=1 \
--chirps_per_sec=4 --gps_sync=5 \
MASTER SLAVE
```

12 Appendix: AD9854 Quickref

Table IV. Register Layout

Parallel Address	Serial Address	AD9854 Register Layout								
Hex	Hex	Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0	Default Value
00	0	Phase Adjust Register #1 <13:8> (Bits 15, 14 don't care)						Phase 1		00h
01	POTW1	Phase Adjust Register #1 <7:0>								00h
02	1	Phase Adjust Register #2 <13:8> (Bits 15, 14 don't care)						Phase 2		00h
03	POTW2	Phase Adjust Register #2 <7:0>								00h
04	2	Frequency Tuning Word 1 <47:40>						Frequency 1		00h
05	FTW1	Frequency Tuning Word 1 <39:32>								00h
06		Frequency Tuning Word 1 <31:24>								00h
07		Frequency Tuning Word 1 <23:16>								00h
08		Frequency Tuning Word 1 <15:8>								00h
09		Frequency Tuning Word 1 <7:0>								00h
0A	3	Frequency Tuning Word 2 <47:40>						Frequency 2		00h
0B	FTW2	Frequency Tuning Word 2 <39:32>								00h
0C		Frequency Tuning Word 2 <31:24>								00h
0D		Frequency Tuning Word 2 <23:16>								00h
0E		Frequency Tuning Word 2 <15:8>								00h
0F		Frequency Tuning Word 2 <7:0>								00h
10	4	Delta Frequency Word <47:40>								00h
11	DFR	Delta Frequency Word <39:32>								00h
12		Delta Frequency Word <31:24>								00h
13		Delta Frequency Word <23:16>								00h
14		Delta Frequency Word <15:8>								00h
15		Delta Frequency Word <7:0>								00h
16	5	Update Clock <31:24>								00h
17	UCR	Update Clock <23:16>								00h
18		Update Clock <15:8>								00h
19		Update Clock <7:0>								40h
1A	6	Ramp Rate Clock <19:16> (Bits 23, 22, 21, 20 don't care)								00h
1B	RRCR	Ramp Rate Clock <15:8>								00h
1C		Ramp Rate Clock <7:0>								00h
1D	7	Don't Care	Don't Care	Don't Care	Comp PD	Reserved, Always Low	QDAC PD	DAC PD	DIG PD	10h
1E	CR	Don't Care	PLL Range	Bypass PLL	Ref Mult 4	Ref Mult 3	Ref Mult 2	Ref Mult 1	Ref Mult 0	64h
1F		CLR ACC 1	CLR ACC 2	Triangle	SRC QDAC	Mode 2	Mode 1	Mode 0	INT/EXT Update Clk	01h
20		Don't Care	Bypass Inv Sinc	OSK EN	OSK INT	Don't Care	Don't Care	LSB First	SDO Active CR [0]	20h
21	8	Output Shape Key I Mult <11:8> (Bits 15, 14, 13, 12 don't care)								00h
22	IPDMR	Output Shape Key I Mult <7:0>								00h
23	9	Output Shape Key Q Mult <11:8> (Bits 15, 14, 13, 12 don't care)								00h
24	QPDMR	Output Shape Key Q Mult <7:0>								00h
25	A SKRR	Output Shape Key Ramp Rate <7:0>								80h
26	B	QDAC <11:8> (Bits 15, 14, 13, 12 don't care)								00h
27	QDACR	QDAC <7:0> (Data is required to be in two's complement format)								0